

### How Safe is ALERIO?

Readings from ALERIO X-Ray Wall Mounted X-Ray compared to AERB/IEC recommendation.




Safety standards are set by AERB & IEC

AERB: Indian regulatory agency for radiation safety

IEC: International standards for x-ray equipment.

What does the Standards say:

*“The leakage radiation from dental x-ray unit shall not exceed 25mR in one hour, when measured at 1 meter from the unit AND the leakage radiation rate shall not be more than 25mR/hr when measured at 1 meter from the unit”*

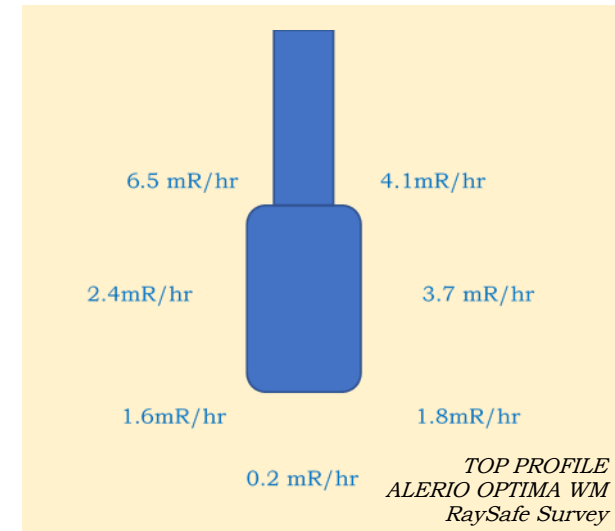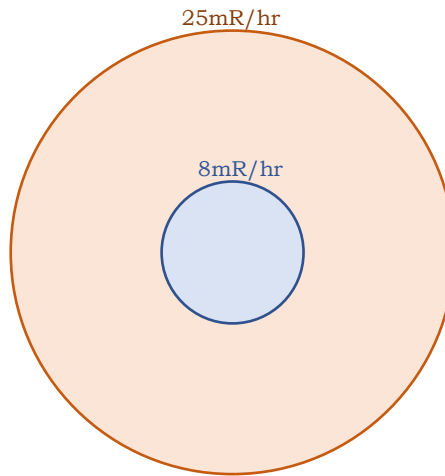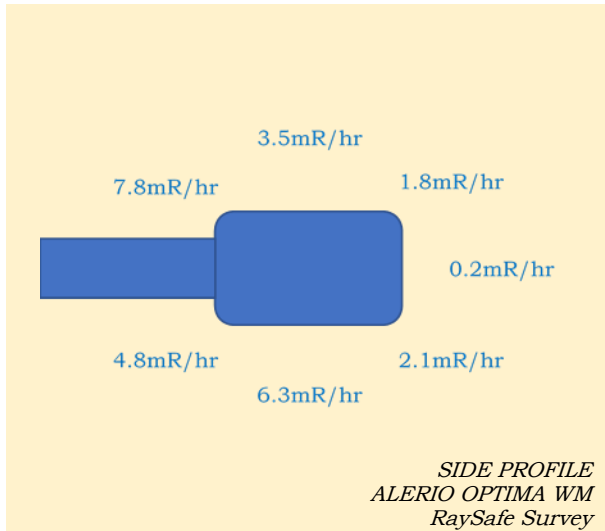

ALERIO X-RAY Leakage Is 66% lower than IEC limits